
# CENTER 302

#### TYPE K J THERMOMETER



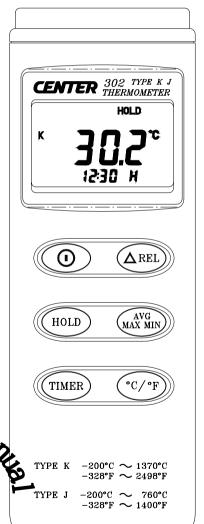

Struction Many

CENTER TECHNOLOGY CORPORATION

## CONTENTS

	TITLE	PAGE
I.	Introduction	1
II.	Specifications	1
Ш	. Symbol Definition and Button Location	3
IV.	Operation Instructions	5
	4.1 Power-Up	5
	4.2 Connection the Thermocouples	5
	4.3 selecting the Temperature Scale	5
	4.4 selecting the Thermocouple Type	5
	4.5 Data-Hold Operation	5
	4.6 Timer Operation	5
	4.7 Relative Operation	6
	4.8 MAX/MIN/AVG Operation	6
	4.9 Auto Power Off	7
	4.10 Low Battery Condition	7
	4.11 Digital output:	7

#### I. Introduction:

This instrument is a digital thermometer for use with any K-type and J-type thermocouple as temperature sensor.

Temperature indication follows National Bureau of Standards and IEC584 temperature/voltage table for K-type and J-type thermocouples.

## II. Specifications:

#### **Numerical Display:**

4 digital liquid crystal display

#### Measurement Range:

```
K-Type -200°C ~ 1370°C
```

-328°F ~ 2498°F

J-Type -200°C ~ 760°C

-328°F ~ 1400°F

#### Resolution:

K-Type:

-328°F~ 1000°F 0.1°F; else 1°F

J-Type:

-328°F~ 1000°F 0.1°F; else 1°F

#### **Maximum Voltage at Thermocouple Input:**

60V DC, or 24Vrms AC

#### **Environmental:**

Operating Temperature and Humidity:

0°C ~50°C (32°F ~ 122°F); 0 ~ 80% RH

☐ Storage Temperature and Humidity:

-10°C to 60°C (14°F ~ 140°F); 0 ~ 80% RH

Altitude up to 2000 meters.

Accuracy: at  $(23 \pm 5^{\circ}C)$ 

Range	Accuracy
K-Type -200°C ~ 1370°C	±(0.1% reading + 0.7°C)
J-Type -200°C ~ 760°C	±(0.1% reading + 0.7°C)
K-Type -328°F ~ 2498°F	±(0.1% reading + 1.4°F)
J-Type -328°F ~ 1400°F	±(0.1% reading + 1.4°F)

#### **Temperature Coefficient:**

For ambient temperatures from 0°C ~ 18°C and 28°C ~ 50°C, for each °C ambient below 18°C or above 28°C add the following tolerance into the accuracy spec.

0.01% of reading + 0.03°C ( 0.01% of reading + 0.06°F )

#### Note:

The basic accuracy Specification does not include the error of the probe please refer to the probe accuracy specification for additional details.

Sample Rate: 3.3 times per second

Dimension: 184×64×30mm

Weight: 210g Approx.

#### Accessory:

K Type Bead Probe, Battery, Carrying Case, Instruction Menu.

#### Option:

Soft Ware Package(Program, RS232 Connection Cable), AC Adapter

### Power requirement:


9 Volt Battery, NEDA 1604 or JIS 006P or IEC6F22

Battery Life: Approx. 100hrs with alkaline battery

AC Adapter: 9Vpc ±15% 100Ma

Plug Diameter: 3.5×1.35mm

# III. Symbol Definition and Button Location:

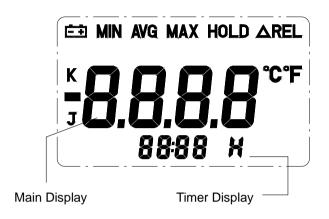

 This indicates that the minus temperature is sensed.

**H** : It indicates that the timer is expressing in hours and minutes.

°C °F : Centigrade and Fahrenheit indication.

**K J**: Thermocouple Type Indication

**HOLD**: This indicates that the display data is being hold.


MAX: The Maximum value is now being displayed


**MIN**: The Minimum value is now being displayed

**AVG**: The Average value is now being displayed.

 $\triangle$ **REL**: The reading is now under Relative Mode.

: The Battery is not sufficient for proper operation.



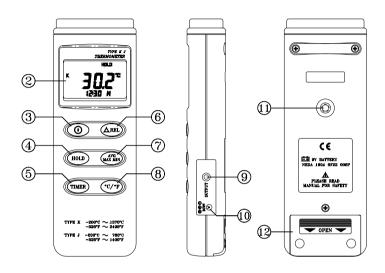

- ① K,J type temperature sensor connector
- ② LCD display
- ③ ON/OFF button
- (4) HOLD button
- 5 Timer function control button
- 6 Relative readout button
- MAX MIN Average control button
- ® °C, °F control button
- 9 Digital output connector
- 10 AC power adapter connector
- 11) Tripod connector
- 12 Battery cabinet cover

## IV. Operation Instructions:

## 4.1 Power-Up

Press the ① key to turn the thermometer On or OFF

## 4.2 Connection the Thermocouples

For measurement, plug the thermocouple into the input connectors.

## 4.3 Selecting the Temperature Scale

When the meter was first power on, the default scale setting is set at Celsius (°C) scale. The user may change it to Fahrenheit (°F) by pressing " °C/°F" button and vice versa to Celsius.

## 4.4 Selecting the Thermocouple Type

By default, when the meter is powered on, it is K-Type, One may press and hold "°**C/**°**F**" button and then power on the meter, then it will change to J-Type.

## 4.5 Data-Hold Operation

The user may hold the present reading and keep it on the display by pressing the "HOLD" button. When the hold data is no longer needed, one may release the data-hold operation by pressing "HOLD" button again. When the meter is under Data Hold operation, the "△REL", (MAX MIN) and " °C/°F" button are disabled.

#### 4.6 Timer Operation:

One may start the timer by press the "**TIMER**" button. The counting can be stopped or continued by pressing it again.

When the counting exceed 59min 59sec, the time scale will be changed to hours and minutes and the "**H**" symbol will appear on the display.

The counting can be reset by press and hold "TIMER" button for 2 sec.

## 4.7 Relative Operation:

When one press the "ARL" button, the meter will memorize the present reading and the difference between the new reading and the memorized data will be shown on the display. Press the "ARL" button again to exit the Relative operation.

#### 4.8 MAX/MIN/AVG Operation:

When one press the (MAX/MIN) button the meter will enter the MAX/MIN mode. Under this mode the maximum value, minimum value and average value of latest 4 data is kept in the memory simultaneously and updated with every new data.

When the MAX symbol is display, the Maximum is shown on the display.

Press (MAX MIN) again, then the NIN symbol is on the display and also the minimum reading.

Press (MAX MIN) again, the AVG symbol is on the display and also the average reading.

Press MAY again, MAX, MIN and AVG will blink together. This means that all these data is updated int the memory and the reading is the present temperature.

One may press (MAX MIN) to circulate the display mode among these options.

When the meter is under (MAX MIN) operation, "△REL" and " °C/°F" are disabled.

To exit the MAX/MIN mode, one may press and hold (MAX MIN) for two seconds.

#### 4.9 Auto Power Off:

By default, when the meter is powered on, it is under auto power off mode. The meter will power itself off after30 minutes if no key operation and RS232 communication. Key combination at power on or RS232 communication can disable auto power off.

One may press and hold "HOLD" button and then power on the meter and there will be two successive beeps to indicate that auto power off is disabled.

### 4.10 Low Battery Condition

When the battery voltage is under proper operation requirement, the symbol will show on the LCD and the battery need to be replaced with new one.


## 4.11 Digital output:

The Digital Output is a 9600bps N 81 serial interface.

The RX is a 5V normal high input port.

The TX is a 5V normal high output port.

The command of Digital Output is list below.

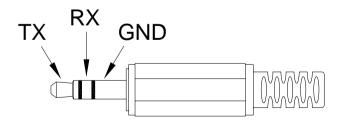

RS232 command	Function	Remarks		
K(ASC 4BH)	Ask for model No.	Send 4 bytes		
D(ASC 44H)	Ask for main display Range, Data, Unit	Send 22 bytes		
B(ASC 42H)	Ask for secondary display Range, Data, Unit	Send 22 bytes		
S(ASH 53H)	Ask Status	Send 13 bytes		
H(ASC 48H)	Hold button			
T(ASC 54H)	TIMER button			
M(ASC 4DH)	AVG/MAX/MIN button			
N(ASC 4EH)	Exit AVG/MAX/MIN mode			
R(ASC 52H)	REL button			
C(ASC 43H)	°C/°F button			
A(ASC 41H)	Inquire all encoded data	Send encoded 8 byte		

#### · Command K:

Return 4 bytes. For example, when sends command "K" to meter, it will return "3","0","2", ASCII(13) .

#### Command D:

Return data of main window.

Range: (unused)

Data: ±9999.9,-OL,OL (7bytes include polarity and decimal point), Unit: C,F(5bytes)

When the meter receive the D command, it will send : Range Data Unit.

( where represent space (ASC(20H) )

For example:

T1 -199.9 C

(0x13) represent T1,- 199.9°C, The total byte number should be 7+1+7+1+5+chr(13)=22Bytes

#### Command B:

Return the counting of timer.

#### Command S:

Return the operation mode HOLD MAX REL, if the mode is not entered, the related characters will be left as space.

For example:

when the meter is under MAX display, the meter will return:

MAX

#### Command T:

Equivalent to one pushing on the HOLD button.

#### · Command M:

Equivalent to one pushing on the HOLD AVG/MAX/ MIN button and no message is returned.

#### · Command R:

Equivalent to one pushing on the REL button and no message is returned.

#### Command C:

Equivalent to one pushing on the  $^{\circ}C/^{\circ}F$  button and no message is returned.

#### · Command A:

#### 1<sup>nd</sup> BYTE:

The first byte is the start byte, it value is 2.

## 2<sup>nd</sup> BYTE:

bit7	bit6	bit5	bit4	bit3	bit2	bit1	bit0
C/F	Low Bat	Hold	REL	K/J	MAX/AVG/MIN		

bit 2	bit 1	bit 0	
0	0	0	→normal mode
0	0	1	→MAXIMUN mode
0	1	0	→MINIMUN mode
1	0	0	→AVG mode
1	1	1	→calculate MAX/MIN/AVG in back-

ground and lcd "MAX""AVG""MIN" will flash.

**bit3:**  $1\rightarrow 0$ ->K TYPE , $1\rightarrow J$  TYPE(300 only has K type)

bit4: 1→REL

bit5: 1→HOLD, 0→not HOLD

bit6: 1→LOW BATTERY, 0→BATTERY NORMAL

**bit7:**  $1 \rightarrow ^{\circ} C \ 0 \rightarrow ^{\circ} F$ 

#### 3<sup>th</sup> BYTE:

bit7	bit6	bit5	bit4	bit3	bit2	bit1	bit0
no use	no use	no use	Time	no use	X1_	minus	OL
			unit		X10		

**bit0:** 1→main window value is OL, 0→not OL

**bit1:** 1→main window value is minus, 0→main window value is plus.

**bit2:**  $1\rightarrow 4^{th}$  byte and  $5^{th}$  byte represent #### ,  $0\rightarrow 4^{th}$  byte and  $5^{th}$  byte represent ###.#

**bit4:** 1→sub window value is MM:SS, 0→sub window value is HH:MM

### 4<sup>th</sup> BYTE:

first two BCD code of main window value.

#### 5<sup>th</sup> BYTE:

last two BCD code of main window value

first two BCD code of sub window value.

### 7<sup>th</sup> BYTE:

last two BCD code of sub window value.



4 / F NO. 415, Jung-Jeng Rd., 238 Shu-Lin Chien, Taipei, Taiwan TEL: 886-2-26763926 E-Mail: center@centertek.com FAX: 886-2-26763925 http://www.centertek.com

302-00



Distributor in Australia
Pacific Sensor Technologies Pty Ltd
Unit 4, 3 Neutron Place Rowville, VIC 3178 Australia
1300 662 720 | sales@pacificsensortech.com.au
www.pacificsensortech.com.au